



FlexiPump™ Independent Flushing System Attaching Adapters

FlexiPump Unit



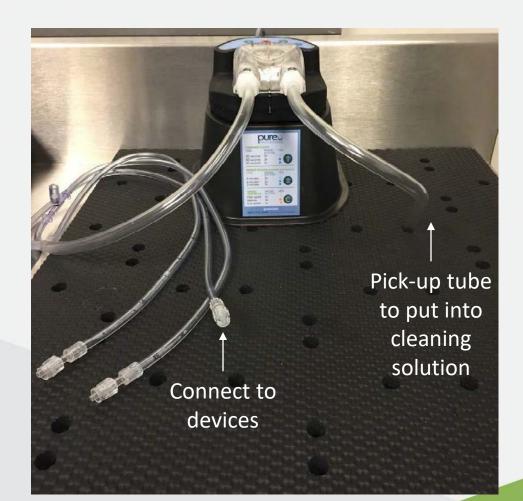


Luer locks

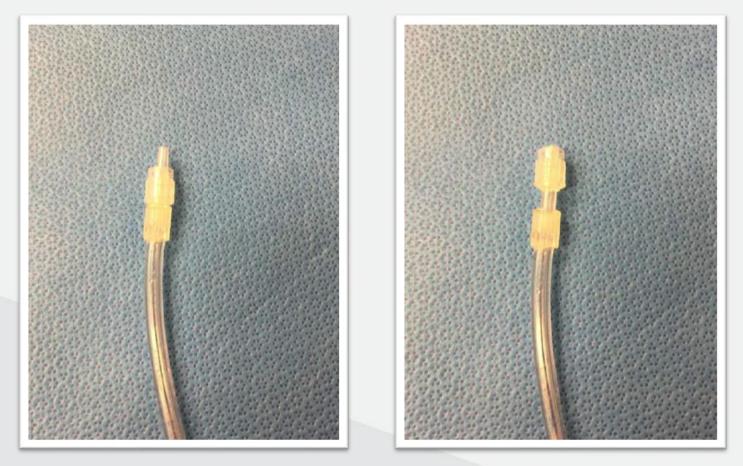



Connecting luer with devices

Easy connection with luer and slip tip

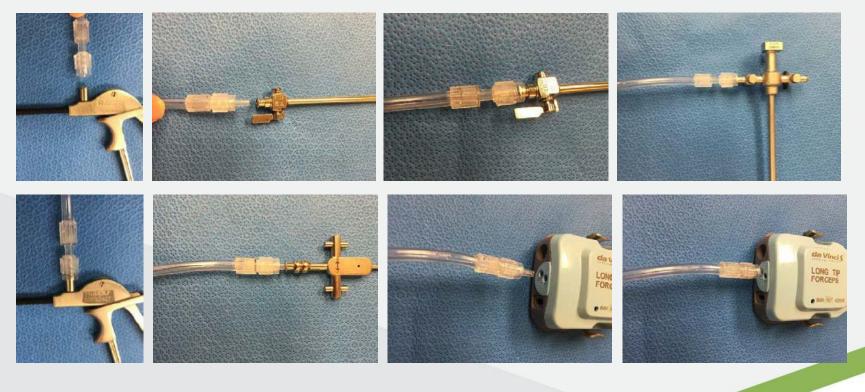



Adapters


Additional adapters available: act as the seal or bridge from the device to tube set on the pump.



XL Slip Tip
Adapter
Product
ID:
XLSLIP-30

Female to Female luer lock Product ID: FFLL-30


Rubber Cup Adapter Product ID: RCA-01







All adapters below act as the seal or bridge from the device to tube set on the pump.

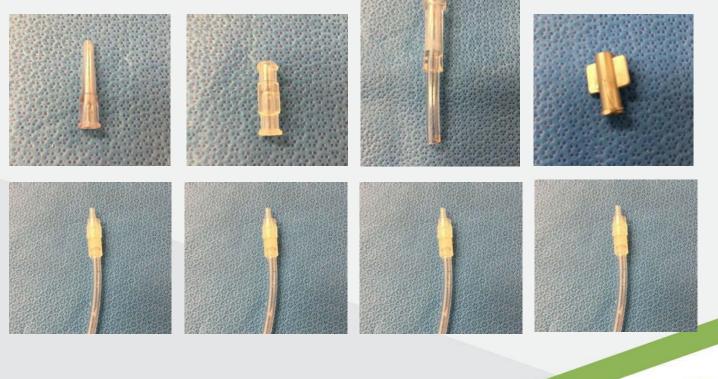



6 Attaching Surgical Devices

Adapters






Flushing robotic ports

• Flush both ports at once; use XL Slip Tip



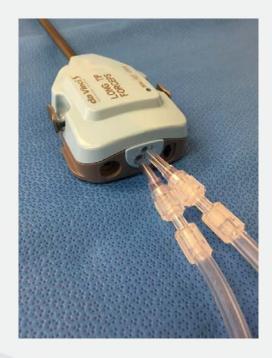

Slip tip into port

Screw in the luer, then flush



Rubber cup adapter



Slide cup adapter over devices end

Slide slip tip into tube end-FLUSH



9 Attaching Surgical Devices

XL Slip Tip



Put XL slip tip into opening on device



Slid, twist to engage lack and get seal from tube set on pump



Female to Female Luer Lock





Screw the female end into device

Screw male end of tube set into female



Attaching Surgical Devices

11

Pure Processing 877.718.6868 www.pure-processing.com sales@pure-processing.com

